

PosiTest® AT Verifier

Instruction Manual v. 2.0



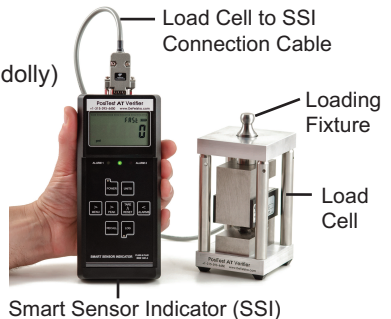
Introduction

The *PosiTest AT Verifier* kit is ideal for checking the accuracy and operation of adhesion testers and is an important component in fulfilling both ISO and in-house quality control requirements.






The kit is ready to use with all *PosiTest* pull-off adhesion testers. All setup information has been preset by DeFelsko. No additional configuration is required or recommended. If the Smart Sensor Indicator (SSI) settings are mistakenly altered, see *Reconfiguring the SSI Device* (pg. 3).

Kit includes:

- Smart Sensor Indicator (SSI) Device
- Load Cell with steel 20mm Loading Fixture (dolly)
- Built-in rechargeable Lithium Ion Batteries
- Universal AC power adaptor/charger
- Instruction Manuals (2)
- Certificates of Calibration (2)
- Sample Certificate of Accuracy
- Measurement Uncertainty Worksheet
- Hard shell carrying case



How to Perform a Test

1. Connect the *PosiTest AT* actuator to the load cell. Ensure the quick coupling is locked in place over the dolly fixture. Ensure all pressure has been released within the adhesion tester by pushing the *PosiTest AT* actuator handle completely down.
 2. Press [Power] button to power-up the Smart Sensor Indicator (SSI).
 3. Press and release the [TARE] button to ZERO the SSI.
 4. Press and release the [PEAK] button to hold the maximum pressure value at the completion of the test. PEAK will display on the SSI.
 5. Power ON the *PosiTest AT* (if OFF) by pressing the green  button.
 - Ensure units are set to psi and dolly size to 20 mm.
 - Important:** *PosiTest AT-A* (automatic) models: Set the pull rate to 30 psi/sec
PosiTest AT-M (manual) models: Close the pressure relief valve
 6. Press the  button to ready the *PosiTest AT*.
 7. Press the  button again to start the test.
 - PosiTest AT-A* models will automatically begin building pressure*
 - PosiTest AT-M* models: slowly prime the pump until the priming pressure is reached (100 psi). Return pump handle to its full upright position and maintain a single slow, continuous pump at approximately 100 psi/sec until a verification point has been reached*.
- *Make no comparisons between PosiTest adhesion tester and SSI measurements until the priming pressure (100 psi) has been exceeded. STOP the test before reaching 3000 psi (highest verification point should be slightly under 3000 psi).*
8. Stop the test when the verification point has been reached.
 - PosiTest AT-A* users press the red  button. Reading will flash and actuator will automatically release pressure.
 - PosiTest AT-M* users simply release the pump handle and open the pressure relief valve (turn counter-clockwise).
 9. Record values from *PosiTest AT* and *Smart Sensor Indicator*.
 10. Prepare for next test verification point.
 - Power-down the SSI by pressing the [Power] button.
 - PosiTest AT-A* only: Hold down the  button for 2 seconds to power-down.
 - Ensure all pressure has been released within the adhesion tester by pushing the *PosiTest AT* actuator handle completely down.

Repeat steps 2-10 for each additional verification point. See included Sample Certificate of Accuracy for recommended verification points.

Verification of Test Results

When verifying *PosiTest AT* Adhesion Tester accuracy, it is recommended that several verification points be tested. See the included Sample Certificate of Accuracy for recommended verification points.

Test results should fall within the combined accuracy of the *PosiTest AT* Adhesion Tester (± 30 psi full scale) and *PosiTest AT Verifier* (pg. 4).

The included Measurement Uncertainty Worksheet and Sample Certificate of Accuracy documents have been pre-populated with data unique to your *PosiTest AT Verifier*.

If any of the verification points are outside of these combined accuracies, the *PosiTest AT* may require recalibration. Contact DeFelsko or your local dealer for information on returning your adhesion tester for recalibration.

Certification

The *PosiTest AT Verifier* includes a Certificate of Calibration for the SSI device and one for the load cell. For information on returning your *PosiTest AT Verifier* for recertification, contact DeFelsko or your local dealer.

The *PosiTest AT Verifier*, with a valid Certificate of Calibration, can be used to check the accuracy of *PosiTest* Adhesion Testers. A sample Certificate of Accuracy is included.

Reconfiguring the SSI Device

The SSI device comes pre-configured for verification of *PosiTest AT-M* and *AT-A* pull-off adhesion testers. No additional configuration is required or recommended.

If the SSI is mistakenly altered, configuration can be restored by following the steps outlined in our *Reconfiguration Guide*.

The guide is available at: defelsko.com/at/verifier/guide.pdf

Technical Specification

Range: 0 - 5,000 psi **Resolution:** 1 psi **Accuracy*:** ± 6.33 psi (± 0.044 MPa)

*Worst case measurement system uncertainty. See included Measurement Uncertainty Worksheet for the actual uncertainty of your kit.

NOTE: Device displays imperial units only.

Conversion Factor:

1 megapascal (MPa) = 145 pounds/inch² (psi)

Returning for Service

If you need to return the *PosiTest AT Verifier* for service, describe the problem fully and include reading results, if any. Be sure to include contact information including your company name, company contact, telephone number and fax number or email address. defelsko.com/support

Limited Warranty, Sole Remedy and Limited Liability

DeFelsko's sole warranty, remedy, and liability are the express limited warranty, remedy, and limited liability that are set forth on its website:
www.defelsko.com/terms.

DeFelsko[®]
The Measure of Quality
www.defelsko.com

© DeFelsko Corporation USA 2017. All Rights Reserved

This manual is copyrighted with all rights reserved and may not be reproduced or transmitted, in whole or part, by any means, without written permission from DeFelsko Corporation.

DeFelsko and PosiTest are trademarks of DeFelsko Corporation registered in the U.S. and in other countries. Other brand or product names are trademarks or registered trademarks of their respective holders.

Every effort has been made to ensure that the information in this manual is accurate. DeFelsko is not responsible for printing or clerical errors.